ALiViON

Welcome to Alivion!

We're thrilled to have you as part of our community. With our calibration bottles, you can easily calibrate your device at any time. Follow the steps outlined here to ensure optimal performance of your device.

Find out more on alivion.ch:
User Manual, Service & Support

Alivion AG Flughofstrasse 42 8152 Glattbrugg Switzerland
+41 41 511 46 71 service@alivion.ch

Getting started

You have purchased a Nutrion™ Calibration Set. Before using it, follow these instructions to ensure proper use.

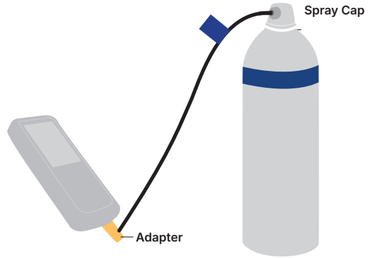

Warning
Use the sample tube with the **BLUE** label only with the **BLUE** labeled *Calibration Standard 1*, and the sample tube with the **YELLOW** label only with the **YELLOW** labeled *Calibration Standard 2*.

Preparation for the calibration

To ensure accurate measurements, you need to calibrate your Nutrion™ every two weeks. The calibration follows a two-point calibration process, meaning you will use two different calibration standards in succession. Your device will notify you automatically when a new calibration is required.

Follow these steps to perform the calibration:

1. Turn on your Nutrion™ device.
2. Go to the device menu and select *Settings → Calibration*.
3. The device will guide you through the individual steps, but make sure to read these instructions carefully.
4. Prepare the calibration standards: Unscrew the metal safety cap from the bottles.
5. Take the two sample tubes out of the packaging.

Warning
Please handle the sample tube with care. Hold only the orange adapter of the Connector when inserting and removing it to the device.

Performing the calibration

Calibration Standard 1

Attach the sample tube with the **BLUE** label to the **BLUE** labeled *Calibration Standard 1*. Gently press the white spray cap onto the bottle valve, as if using a spray can. Insert the sample tube's orange adapter into the Nutrion™ opening where the mouthpiece normally goes. Once secure, follow the Nutrion™ instructions.

As soon as everything is connected and the Nutrion™ screen tells you to press the Spray Cap, do so by pressing it vertically down and hold it.

The screen will then display a timer counting down. Once the timer ends, release the Spray Cap immediately. The device will now execute the first part of the evaluation.

Calibration Standard 2

While the device is processing the first calibration, prepare for the second calibration: Connect now the sample tube with the **YELLOW** label to the **YELLOW** labeled *Calibration Standard 2* and the Nutrion™ device. Once the device is ready, you will be prompted to press the Spray Cap and repeat the procedure described for the blue *Calibration Standard 1*.

For more information, refer to the Nutrion™ User Manual at alivion.ch.

Storage

Please ensure that the Calibration Standards are not exposed to direct sunlight and never heat up above 50 °C. The sample tubes can remain on the bottles during storage.

At the end of its life, do not dispose of this product as regular waste. Instead, dispose of it at a disposal point for the recycling.